





PROCEDURE FOR FELINE MINOR CROSSMATCH

Material provided: 10 gel tests 2 buffer solutions 1 rack for gel tests


Sample material: RECIPIENT packed RBCs; DONOR serum or plasma.


Further material required: Centrifuge with swinging bucket; micropipette; 2 test tubes.

MANDATORY EQUIPMENT: Use only swinging bucket centrifuge.

N°1: Centrifugation of the gel test before use


Centrifuge the gel test for 2 minutes at 1000g (if you are using «RPM» unit, please contact us), without dissociating the gel test tube from the gel test support. DO NOT FORGET TO ADD A BALANCE.

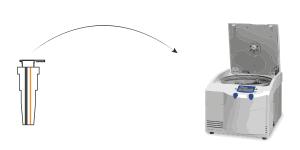

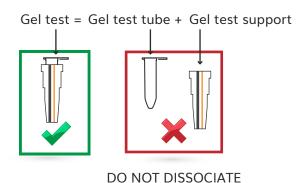

N°2: Preparation of blood samples for Minor XM







DONOR Centrifuge blood tube in order to collect serum or plasma. Serum or plasma

Blood sample specification:

- EDTA / ACD / CPD / Plain tube
- Do not use Heparin

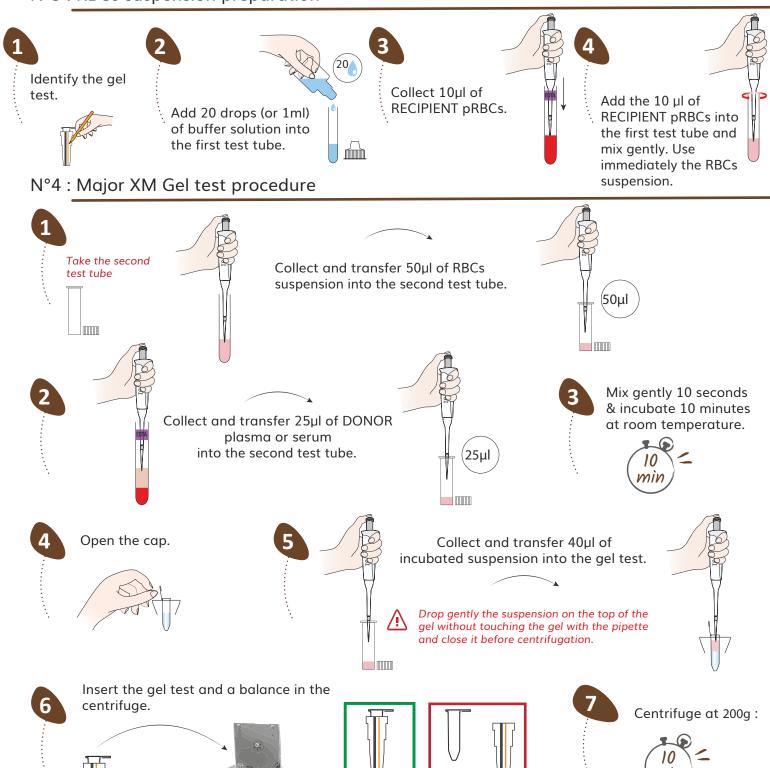

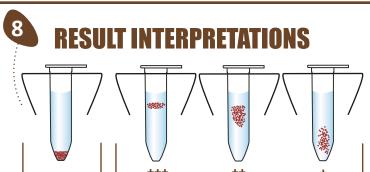

Incompatibility

Do not Transfuse

Compatibility

Safe transfusion

/ J

DO NOT DISSOCIATE FOR CENTRIFUGATION

Troubleshooting:
Please contact the
Scientific Service Laboratory
contact@alvedia.com
+33(0)478 380 239

